



This is to certify that

## LABORATORIO ACLIMU

Has participated in the following  
SmartSpot Quality Proficiency Testing  
for 2022

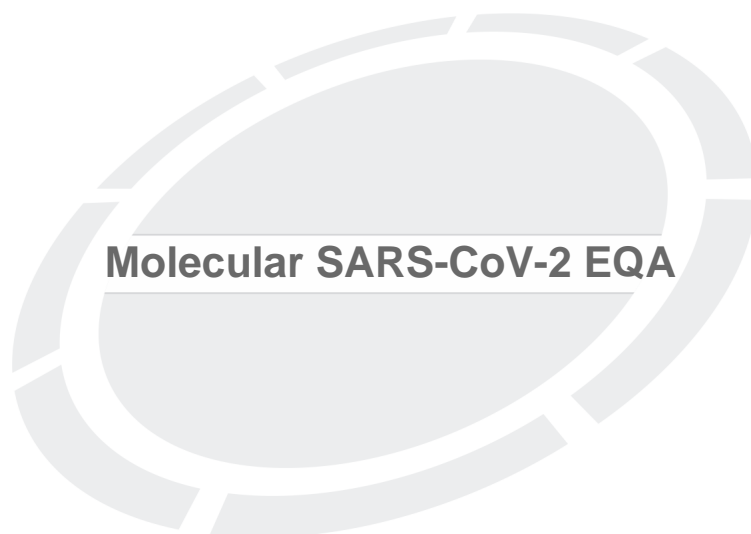

and achieved the following scores for  
Instrument 785BR24344

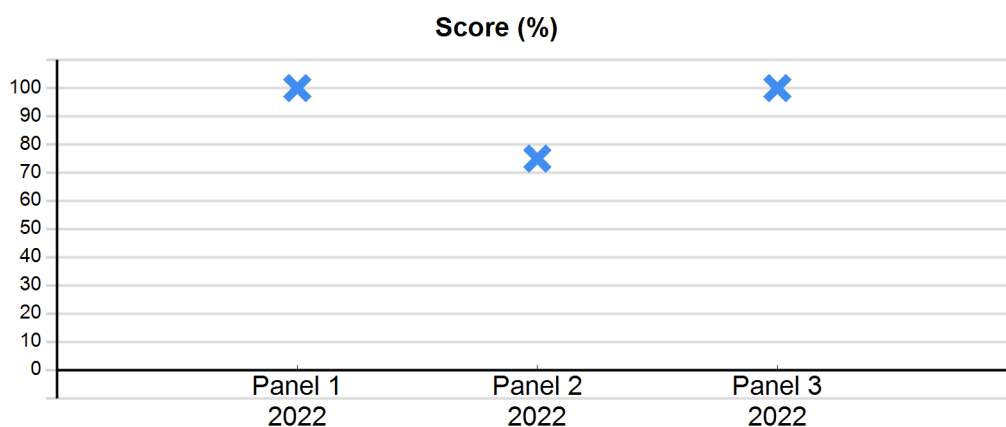

2023/06/12

Scheme Coordinator

Date

[Anest@SmartSpotQ.com](mailto:Anest@SmartSpotQ.com)